Using Optical Flow Fields for Polyp Detection In Virtual Colonoscopy

Burak Acar¹, Sandy Napel¹, David Paik¹, Burak Göktürk², Carlo Tomasi³, and Christopher F. Beaulieu¹

Stanford University, Department of Radiology
 LUCAS MRS Center, 3D Lab., Stanford, CA 94305-5488, USA bacar, snapel @stanford.edu
 paik@smi.stanford.edu, cfb@s-word.stanford.edu
 URL: www.3dradiology.org
 Stanford University, Electrical Engineering Department Stanford, CA 94305, USA
 Stanford University, Computer Science Department Stanford, CA 94305, USA

Abstract. Since the introduction of Computed Tomographic Colonography (CTC), research has mainly focused on visualization and navigation techniques. Recently, efforts have shifted towards computer aided detection (CAD) of polyps. We propose a new approach to CAD in CT images that attempts to model the way a radiologist recognizes a polyp using optical flow fields (OFF). Features extracted from OFFs are used in a linear classifier for polyp detection. An initial validation of our technique resulted in an average of 85% sensitivity and 80.5% specificity in a 10-fold cross validation study on a set of 220 polyp-like structures, 20 of which were true polyps.

1 Introduction

Computed Tomographic Colonography (CTC) was suggested in early 1980's and realized in the 1990's as a minimally invasive method that would make mass screening of colorectal cancer feasible [1–4]. Since then several studies were conducted to assess the performance of CTC [5-10]. In almost all studies, CTC was based on the examination of CT images by an expert radiologist, using either the 2D images, 3D virtual colonoscopic views or both. Thus, until recently most efforts were directed towards developing better visualization and navigation techniques [4,11–19]. Lately, more effort has been put into computer aided detection (CAD), whose ultimate goal is to identify polyps in a 3D CT data efficiently, and with high sensitivity and specificity. Mir et al. reviews a set of techniques that can be used for shape description in CT images [20]. We are aware of two studies on CAD in CTC: Summers et al. reported a shape based polyp detector and concluded that CAD is feasible in CTC [21] and Paik et al. proposed a Hough Transform-based polyp detector [22, 23]. However, these CADs suffer from low specificity, which would require radiologists to examine a large number of CAD hits to rule out false detections.

The goal of our research is to develop a highly sensitive and specific CAD for CTC. We attempted to model the way a radiologist recognizes a polyp by focusing on the changes in consecutive images as one scrolls back and forth in the 3D data. We used Optical Flow Fields (OFF) to represent these changes, and a linear classifier acting on these features to recognize true polyps.

2 Method

2.1 Data Acquisition

Patients were imaged in supine position after colon cleansing and air-insufflation of the colon on a GE HiSpeed Advantage single detector or GE LightSpeed multirow detector scanner (GE Medical Systems, Milwaukee, WI). Typical acquisition parameters were 3 mm collimation, pitch 1.5-2.0, 1.5 mm reconstruction interval, 120 KVp, 200 MAs for the single detector scanner and 2.5 mm collimation, pitch 3.0, 1.0-1.5 mm reconstruction interval, 120 KVp, 56 MAs for the multirow detector scanner. Data were stored as 2 byte unsigned integers. The size of the 3D data matrix was $512 \times 512 \times N$, N is the number of axial slices. N is typically around 350. The average voxel size was $0.74mm \times 0.74mm \times 1.31mm$.

2.2 Initial Detection

The data was preprocessed by a Hough Transform based polyp detector (HTD) [22,23]. HTD basically computes the normals to an isointensity surface and searches for voxels at which a large number of normals intersect. Defining the number of normals that intersect in a given voxel as the HT score of that voxel, a threshold is applied for detection. Typically the voxels at the centers of spherical structures have high scores. The detected voxels mark the locations of polyps with high sensitivity but low specificity. We extracted a subvolume consisting of $21 \times 21 \times 21$ voxels centered on each detection with a score above a fixed threshold.

2.3 Optical Flow Field Computation

The aim of the OFF computation is to characterize the change in the location of the edges (tissue/air boundary) in the image plane while scrolling back and forth along the third dimension. This third dimension can be thought as the time axis [24]. If we name the image plane as the xy-plane then the basic optical flow equation is [25]:

$$\nabla I.\mathbf{v} + \frac{\partial I}{\partial t} = 0 \tag{1}$$

where $\mathbf{v}(x,y)$ is the OFF and I(x,y) is the image, i.e. the intensity function. Equation 1 allows only the computation of \mathbf{v}_{\perp} , the component along the local ∇I . This serves to our purpose and it is simple. We will refer to \mathbf{v}_{\perp} as \mathbf{v} in what follows.

Keeping in mind that the coordinates of the voxel detected by HTD (HT_hit) is (0,0,0), $\mathbf{v}_t(x,y)$ is computed for $x,y,t\in[-10,10]$. t is first incremented from 0 to 10 and then from 0 to -10. This is equivalent to moving outwards from the center. This assures the consistency in the direction of motion of the edges of spherical structures. $\mathbf{v}_t(x,y)$ are summed and the resulting OFF is filtered with a moving average filter of window size of 3×3 cells as

$$\mathbf{v}_{i}(x,y) = Moving_Average\left(\Sigma_{t}\mathbf{v}_{t}(x,y)\right), i \in X, Y, Z$$
(2)

Each $\mathbf{v}_i(x,y)$ corresponds to scrolling along the direction i.

2.4 Optical Flow Field Characterization

The OFF characterization starts with the detection of the parent and the child nodes. The parent node is defined to be the minimum divergence point in the vicinity ($\pm 2 \ cells$) of the HT_hit. This is the most likely location of the center of a polyp. The child nodes are defined to be the points on the incoming streamlines, 5 units away from the parent node. There are 8 child nodes, each corresponding to a streamline ending at a different immediate neighbor of the HT_hit.

A topology based quantitative characterization of the $\mathbf{v}_i(x,y)$, $i \in X, Y, Z$, at the parent node, is employed. It is represented as a point on the 2D $\alpha\beta$ -plane, where α and β are defined as follows [26]. Let

$$\mathbf{J} = \begin{bmatrix} \frac{\partial v_x}{\partial x} & \frac{\partial v_x}{\partial y} \\ \frac{\partial v_y}{\partial x} & \frac{\partial v_y}{\partial y} \end{bmatrix}, \tag{3}$$

$$P = -trace(\mathbf{J}),\tag{4}$$

$$Q = |\mathbf{J}|,\tag{5}$$

then

$$\alpha = P,\tag{6}$$

$$\beta = sign(P^2 - 4Q)\sqrt{|P^2 - 4Q|}. \tag{7}$$

 α and β essentially carry the information present in the eigenvalues of the characteristic equation

$$\lambda^2 + P\lambda + Q = 0 \tag{8}$$

They depend on the local divergence, curl and magnitude of the OFF. The origin of the $\alpha\beta$ -plane corresponds to a uniform OFF.

As the third feature, the angular spread of the locations of child nodes around the parent node is defined as

$$d = \frac{1}{8} \Sigma_i \left(\frac{1}{7} \sqrt{\Sigma_j \theta_{ij}^2} \right) , \theta_{ij} = \angle(child_i, child_j) \in [0, \pi],$$
 (9)

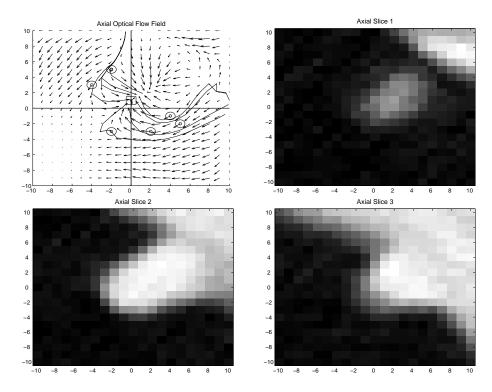


Fig. 1. 3 axial images and the axial OFF. The parent node is marked with a small square and the child nodes are marked with small circles. 3 of the 8 child nodes are coincident.

taking the parent node as the origin. Larger d's indicate increased spread of the child nodes around the parent node.

The 3D feature vector, $[\alpha \ \beta \ d]$, is computed for all three $\mathbf{v}_i(x,y)$, $i \in X,Y,Z$. The median value for each feature is used in the final 3D feature vector used for classification. Figure 1 shows three axial images of a polyp, corresponding to three different t values (the image plane is the axial plane) and the computed OFF associated with this t-axis ($t \equiv z$).

3 Analysis

Data were acquired from 8 patients (7 male and 1 female with age 41-85, mean age 63) as described in Section 2.1. Preprocessing with a HT score threshold of 10000 resulted in 220 HT_hits. Fiber optic colonoscopy results showed that 7 patients had a total of 20 polyps and that all polyps were detected by HTD. This means that the HTD had 100% sensitivity but a large number of false positives. These 220 HT_hits were used as inputs to our algorithm.

Experiment #	Sensitivity	Specificity
1	2/2	13/20
2	2/2	15/20
3	2/2	17/20
4	2/2	17/20
5	2/2	16/20
6	1/2	17/20
7	2/2	11/20
8	2/2	18/20
9	1/2	18/20
10	1/2	19/20
Mean	85%	80.5%

Table 1. 10-fold cross validation results on a set of 220 HT_hits (20 true polyps).

We divided the data set into 10 equal size subsets randomly, such that each subset contains 2 true positive and 20 false positive HT_hits. Nine of these subsets were used for training and the remaining one was used for testing in a 10-fold cross validation study. We used the built-in linear discriminant classifier function (classify.m) of MatlabTM (The MathWorks, Inc., MA, USA). This function minimizes the Mahalanobis distance between the learning and testing feature vectors [27]. The Mahalanobis distance, r, between two vector \mathbf{a} and \mathbf{b} is defined as

$$r_{\mathbf{a}\mathbf{b}}^2 = (\mathbf{a} - \mathbf{b})^T \mathbf{C}^{-1} (\mathbf{a} - \mathbf{b})$$
, where **C** is the covariance matrix. (10)

We had an average sensitivity of 85% and a specificity of 80.5% over 10 tests performed. Table 1 shows the individual sensitivity and specificity results of the cross validation experiments.

4 Discussion

Our ultimate goal is to decrease the radiologists' reading time by directing them towards the true polyps. To do this, we model the way a radiologist recognizes a polyp in 3D CT data based on the motion of edges as one scrolls back and forth through parallel planes transecting a suspicious structure. It is obvious that the choice of scrolling direction affects the computed OFF. We tried to decrease this dependency by performing the analysis in three orthogonal directions and using the median values of each feature. A more robust approach would be to use multiple scrolling directions and construct a feature vector out of the histograms of measured feature values. Using additional features, like the homogeneity of the region of interest, might also improve performance.

Our method is aimed to improve the HT-based CAD results by increasing the specificity. However, it can also be used to detect polyps directly from the 3D CT data without the need for the HTD. The OFFs associated with different scrolling directions can be computed for the whole volume and then CAD can be performed in the vicinity of the colon, based on α , β and d values.

The classifier we used performs linear discriminant analysis based on the minimization of the Mahalanobis distance between the learning and the test samples. The advantages of using the Mahalanobis distance are: (i) It automatically accounts for scaling, (ii) it takes care of the correlation between features and (iii) it can provide linear and curved decision boundaries. Another possible classifier would be the Support Vector Machines (SVM) [28]. SVMs are capable of trading off the training error with the generalization error. They can work practically in infinite dimensional feature spaces. The choice of the parameters and the feature space is critical for SVMs' performance and is the subject of future work.

5 Conclusion

We showed that the idea of modeling the way a radiologist recognizes polyps in 3D CT data is feasible. Optical flow fields (OFF) provide a robust framework for quantitative analysis of inter-slice relations in the 2D CT images. Although many different features can be extracted from OFFs, we showed that α , β and d carry relevant information for polyp recognition. However, several other features may be useful to obtain better performance. Further research is required to optimize the feature space and the classifier.

References

- 1. Coin, C.G., Wollett, F.C., et al.: Computerized radiology of the colon: a potential screening technique. Comput. Radiol. **7(4)** (1983) 215–221
- Chaoui, A.S., Blake, M.A., et al.: Virtual colonoscopy and colorectal cancer screening. Abdom. Imaging 25(2) (2000) 361–367
- 3. Johnson, C.D., Dachman, A.H.: CT colonography: the next colon screening examination? Radiology 216(2) (2000) 331-341
- Vining, D.J.: Virtual colonoscopy. Gastrointest. Endosc. Clin. N. Am. 7(2) (1997) 285–291
- Hara, A.K., Johnson, C.D., et al.: Detection of colorectal polyps by computed tomographic colography: feasibility of a novel technique. Gastroenterology 110(1) (1996) 284–290
- Macari, M., Milano, A., et al.: Comparison of time-efficient CT colonography with two- and three-dimensional colonic evaluation for detecting colorectal polyps. Am. J. Roentgenol 174(6) (2000) 1543-1549
- 7. Hara, A.K., Johnson, C.D., et al.: Detection of colorectal polyps with CT colography: initial assessment of sensitivity and specificity. Radiology **205(1)** (1997) 59–65
- 8. Rex, D.K., Vining, D., et al.: An initial experience with screening for colon polyps using spiral CT with and without CT colography. Gastrointest. Endosc. **50(3)** (1999) 309–313

- ASGE, American Society for Gastrointestinal Endoscopy: Technology status evaluation: virtual colonoscopy: November 1997. Gastrointest. Endosc. 48(6) (1998) 708-710
- Dachman, A.H., Kuniyoshi, J.K., et al.: CT colonography with three-dimensional problem solving for detection of colonic polyps. Am. J. Roentgenol 171(4) (1998) 989-995
- Paik, D.S., Beaulieu, C.F., et al.: Visualization modes for CT colonography using cylindrical and planar map projections. J. Comput. Assist. Tomogr. 24(2) (2000) 179-188
- 12. Kay, C.L., Kulling, D., et al.: Virtual endoscopy comparison with colonoscopy in the detection of space-occupying lesions of the colon. Endoscopy **32(3)** (2000) 226–232
- 13. Lee, T.Y., Lin, P.H., et al.: Interactive 3D virtual colonoscopy system. IEEE Trans. Inf. Tech. Biomed. 3(2) (1999) 139–150
- Beaulieu, C.F., Jeffrey, Jr., R.B., et al.: Display modes for CT colonography. Part II. Blinded comparison of axial CT and virtual endoscopic and panoramic endoscopic volume-rendered studies. Radiology 212(1) (1999) 203-212
- Wang, G., McFarland, E.G., et al.: GI tract unraveling with curved cross sections. IEEE Trans. Med. Imaging 17(2) (1998) 318-322
- McFarland, E.G., Brink, J.A., et al.: Visualization of colorectal polyps with spiral CT colography: evaluation of processing parameters with perspective volume rendering. Radiology 205(3) (1997) 701-707
- 17. Haker, S., Angenent, S., et al.: Nondistorting flattening maps and the 3D visualization of colon CT images. IEEE Trans. Med. Imaging 19 (2000) 665-670
- Paik, D.S., Beaulieu, C.F., Jeffrey, R.B., Rubin, G.D., Napel, S. Automated flight path planning for virtual endoscopy. Med. Phys. 25(5) (1998) 629-637
- Samara, Y., Fiebich, M., Dachman, A.H., Kuniyoshi, J.K., Doi, K., Hoffmann, K.R. Automated calculation of the centerline of the human colon on CT images. Acad Radiol. 6(6) (1999) 352-359.
- Mir, A.H., Hanmandlu, M., et al.: Description of shapes in CT images. IEEE EMBS Mag. 18(1) (1999) 79–84
- Summers, R.M., Beaulieu, C.F., et al.: Automated polyp detector for CT colonography: feasibility study. Radiology 216(1) (2000) 284-290
- Paik, D.S., Beaulieu, C.F., et al.: Computer aided detection of polyps in CT colonography: free response ROC evaluation of performance. Radiological Society of North America 86th Scientific Sessions, Chicago, IL, November, 2000.
- Paik, D.S., Beaulieu, C.F., et al.: Detection of polyps in CT colonography: a comparison of a computer aided detection algorithm to 3D visualization methods. In: Proc. Radiological Society of North America 85th Scientific Sessions, Chicago, IL, November, 1999.
- Yiu-Fai, W., Tsuhan, C.: Compression of medical volumetric data in a video-codec framework. ICASSP 4 (1996) 2128–2135
- Beauchemin, S.S., Barron, J.L.: The computation of optical flow. ACM Computing Surveys 27(3) (1995) 433-467
- Lavin, Y., Batra, R., Hesselink, L.: Feature comparisons of vector fields using earth mover's distance. In: Proc. IEEE/ACM Visualization'98, North Carolina, October, 1998
- 27. Mahalanobis, P. C.: On the generalized distance in statistics Proc. Natl. Institute of Science of India, 12 (1936) 49-55
- 28. Vapnik, V.N.: The nature of statistical learning theory. New York: Springer, 1995